


**Supplementary Figure S1.** Reactivity of rodent samples using strip immunoassay. Seropositive samples are labeled with “+” (A); negative control (NC) and positive control (PC) are shown in (B).

**A**



**B**

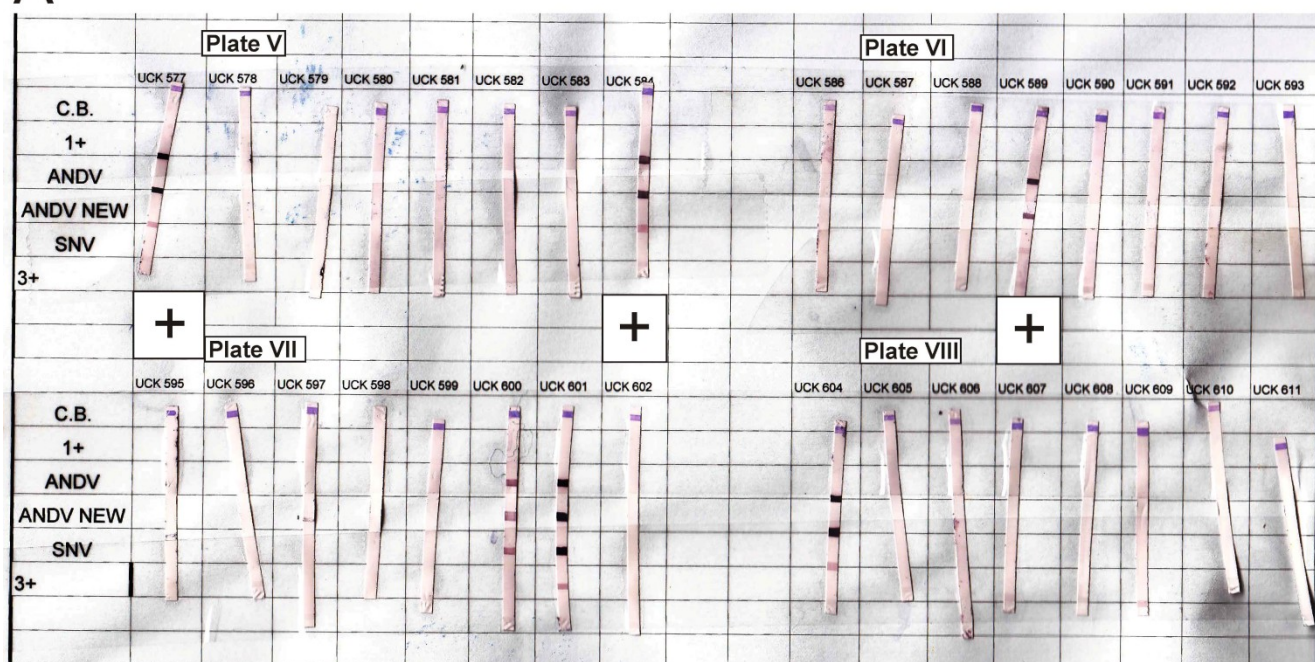